



Emergency Microscope Light Modification by External Source in Absence of Power Supply

Forman Erwin Siagian ^{a*}

^a Department of Parasitology, Faculty of Medicine, Universitas Kristen Indonesia, Jakarta, Indonesia.

Author's contribution

Author FES solely conduct the whole study from designed the study, performed the analysis, wrote the protocol, and wrote the first draft of the manuscript until the final manuscript.

Article Information

DOI: 10.9734/IJPR/2024/v13i1268

Open Peer Review History:

This journal follows the Advanced Open Peer Review policy. Identity of the Reviewers, Editor(s) and additional Reviewers, peer review comments, different versions of the manuscript, comments of the editors, etc are available here: <https://www.sdiarticle5.com/review-history/111418>

Method Article

Received: 17/10/2023

Accepted: 24/12/2023

Published: 04/01/2024

ABSTRACT

Introduction: Microscope is an instrument for visualizing fine detail of an object so that observer can observe the object being examined in detail. The object of examination vary from cells (normal or pathologic), microorganism (such as parasite and bacterium), and even non biological part. There are several types of microscope, one of the oldest forms and still used today is the light microscope. A light microscope relied on continuous light source to operate. The most common source for today's microscopes is an incandescent tungsten-halogen bulb, which is solely electric dependent, positioned in a reflective housing that projects light through the collector lens and into the sub-stage condenser. Current situations sometimes require readiness for conducting microscopic examination anytime, anywhere. Unfortunately, problem occur if the electricity goes out, most people will not be able to continue their microscopic observations. This problem raises the question of what if in an emergency it is necessary to carry out a microscopic examination but unfortunately there is no power source. Below we propose emergency modification efforts so that the microscope can still be used even in conditions without a power source.

Aims: to modify an electric light microscope in such a way that it can continue to be used in the absence of an electrical power source using external source of light.

*Corresponding author: Email: forman.siagian@uki.ac.id;

Discussion: Adding an external source of light is a brilliant approach in order to make the electric dependent light microscope still useable in emergency condition.

Conclusion: it is possible to modify an electric light microscope in the condition of no electric source available and make it operable.

Keywords: Emergency lamp; positioning; lenses; objective; ocular; magnification; light emitting diode.

1. INTRODUCTION

The light microscope is an apparatus for apprehending excellent detail of an object being observed [1,2]; by accomplishing a detailed and enlarged portrayal through the use of a sequences of glass lenses [3], which initially adjust a beam of light onto or through an object or section of an object, and flowed thru convex objective lenses to aggrandized the picture captured [4]; in other word, that it accommodates a two-dimensional aggrandized figure of the specimen being observed [3]. In the majority of light microscopes, the image is viewed instantaneously via binocular eyepieces [5] that act as a secondary lens in the form of a magnifying glass to observe the projected image [2,4]. Such apparatus are named 'compound microscopes' [6]. The term magnification means the microscope's ability to make small objects seem larger, such as making a microscopic organism visible [1,2,6-8]. The total magnification is the sum of the objective magnification (can be 5x, 10x, 40x or 100x) multiplied with the eyepiece magnification (usually 10x) [2,7]. The magnification range extends from $\times 10$ to $\times 1000$, with a resolving power of the order of $0.2 \mu\text{M}$, depending on the type and numerical aperture (area available for passage of light) of the objective lenses.

Common and regular light microscope rely on light produced from lamp which generated electrically to operate [2,6,8]. The most frequent source for nowadays microscopes is an incandescent tungsten-halogen bulb, which is solely electric dependent, positioned in a reflective housing that projects light through the collector lens and into the sub-stage condenser [5,6].

Sometimes in an unexpected situations, emergency microscopic examination needed. Unfortunately, real problem occur when there is no electricity available, and for most people, it will prevent them from doing microscopic observations [9,10]. This problem actually triggers question regarding whether there is an alternative modification that allows observations

to still be carried out in conditions without electricity.

Below we test the emergency modification efforts so that the light microscope can still be used properly, even in conditions without an electric power source. This method is applicable in the field, e.g., when doing field trip, or in limited resources setting.

2. METHODOLOGY

This approach was developed and perfected during the time of laboratory work in the department of Parasitology, Faculty of Medicine, Universitas Kristen Indonesia, Jakarta-Indonesia. We have set a scenario as if it is necessary to carry out a microscopic examination when there is no electrical power source (for example during a power outage).

For the purpose of observation, we prepare light Microscope Olympus CX21 and three Parasitology positive slides of: (1) *Pediculus humanus capitis*, or the head louse, an obligate ecto parasite of man; (2) positive thin blood smear of *Plasmodium vivax*, a hemosporozoan parasite and (3) positive fecal smear of *Entamoeba histolytica* (2 nuclei cyst form). We use combination of bigger object (*Pediculus humanus capitis*) that can easily be seen ini 10×10 or 10×40 magnification with the smaller *P. vivax* and *E. histolytica* that must use 10×100 magnification.

This approach only needed emergency lamp or flashlight from hand phone which is used as a substitute of light source. We use two kind of emergency lamp purchased in a local retail store with specification as follow: the first is a China made APA brand LED 6 watt (32 pcs) white grey emergency lamp equipped with 4V 1600mAh battery, with charging time 12-15 hours, duration of use ~up to 4 hours, 220-240 V/50-60 Hz with dimension $5.26\times 6.3\times 19\text{cm}$ and the second a LED head lamp PowerLite brand LED 3 watt 120 lumen that use three AAA battery 1,5V and the third is using flashlights from a Samsung A 23 phone cell with Li-Po 5000 mAh, non-removable and charging: 25 W wired, LED flash with

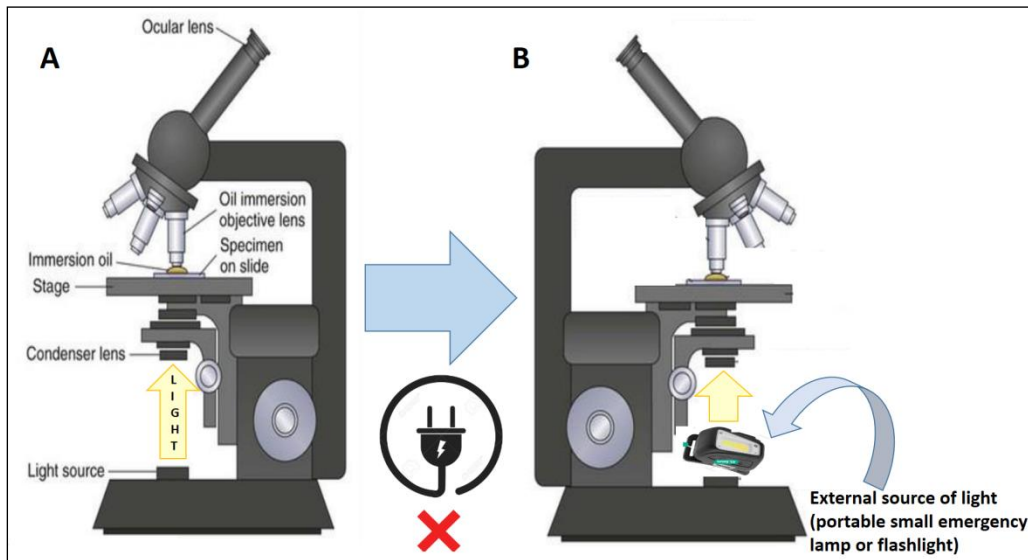


Fig. 1. Schematic part of light microscope.⁷ with modification (A) regular light microscope with its part, (B) simple modification in case there is no electricity available, it is possible to add external light source via emergency lamp or flashlight

adjustable brightness. The author disclaimer that any product or device being used in the test are the author's personal individual experiences, reflecting real life experiences. The authors did not receive support from any organization for the submitted work; and all the device used are the author's personal belonging (except for the microscope and the slide).

3. RESULTS AND DISCUSSION

As its name implies, the light microscope necessitates sufficient light source, which produces light that can be focused, by a

condenser lens, onto the sample [8]. The light that illuminates the specimen reaches a lens known as the objective lens, which creates a magnified image that is inverted, or turned upside down [3].

The method being proposed is simple but substantive modification to existing methods. If an electricity power failure scenario occurs, this simple experiment is aimed at replacing the light source from the lamp pre-installed in the microscope with an external light source, in this case an emergency light or cell phone flashlight.

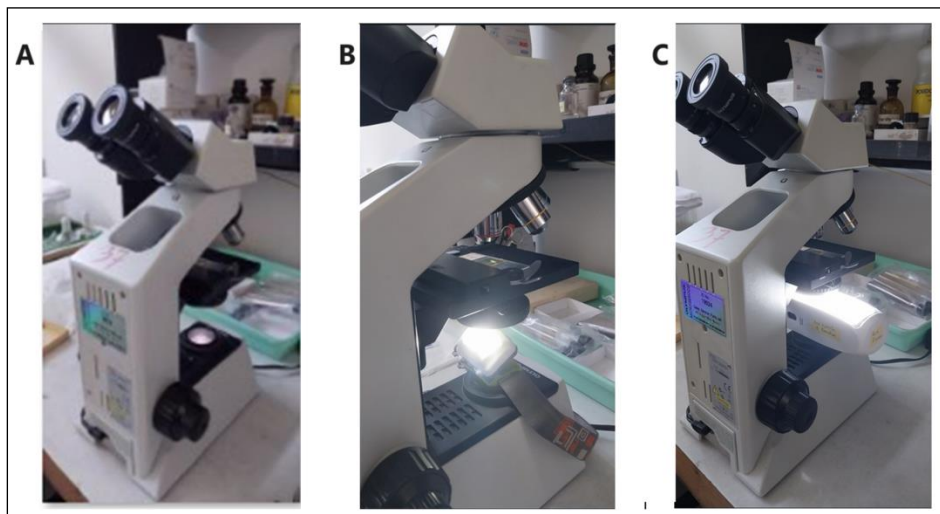


Fig. 2. (A) regular light microscope, (B) light microscope with external emergency head lamp, (C) microscope with external portable emergency lamp (small size)

To my experience, external source of light very likely to be used and applicable in the condition of no electricity. From the point of view of installation, external head lamp and portable emergency lamp (small size) is the easiest and most convenient to use because users only need to place it on the surface of the existing non-operable lamp and customarily do not require plenty of adjustment. Once it has settled and turned on, all that needs to be done is to make adjustments on the microscope examination table, as is usually done on microscopes in normal working conditions. The output of this

small LED emergency lamp is around 6W, and is estimated equal to 400 lumens [11].

All picture in Fig. 3 actually taken in non-standar condition (using external light source) actually showed remarkable result. Eventhough in terms of lighting quality, there is a slight defect in the photo taken using a headlamp as the light source that it seems to have a slightly green tint when compared to those taken using a small emergency lamp. In my opinion, emergency lamp produces a more natural light compared to head lamp.

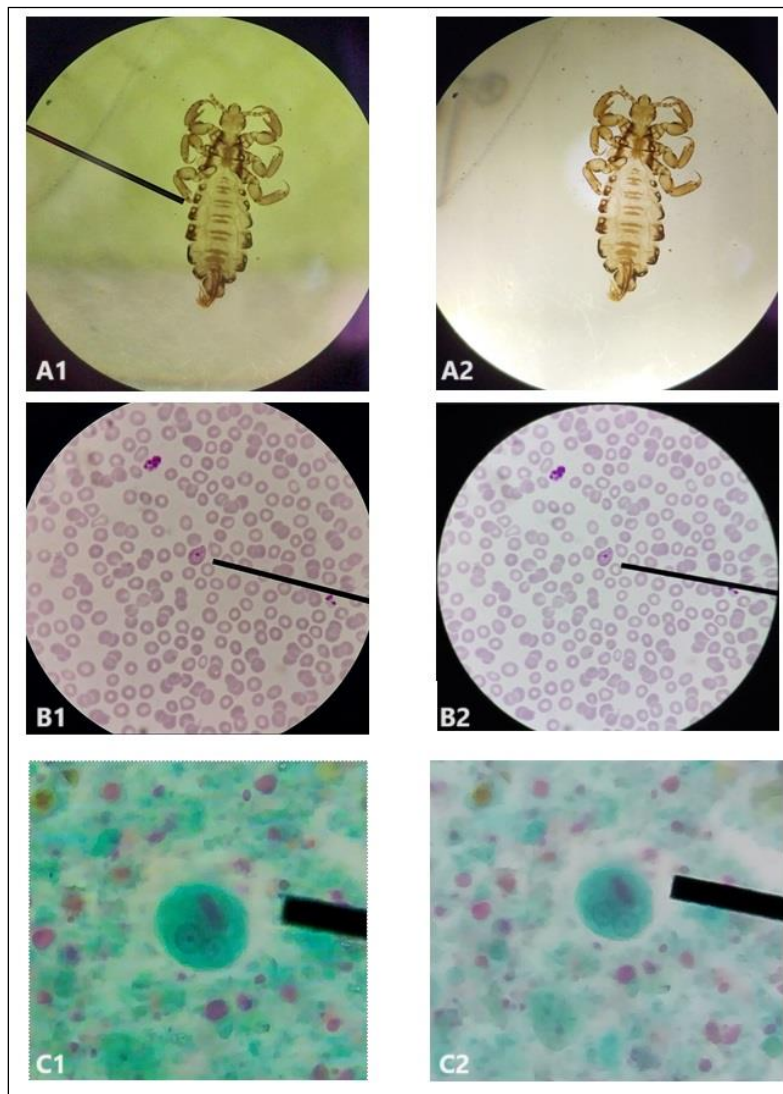


Fig. 3. Comparison of parasitic agent taken with cell phone using external emergency head lamp (all the picture with number 1) and small size emergency lamp (all the picture with number 2). (A) *Pediculus humanus capitis* (magnification 10x10), (B) *Plasmodium vivax* mature trophozoite (amoeboid form) (magnification 10x100), (C) *Entamoeba histolytica*, cyst form with two nuclei (all slides are courtesy of dept. of Parasitology, Faculty of Medicine, Universitas Kristen Indonesia, Jakarta-Indonesia)

These findings reveal that external lights can be used as an alternative light source, when there is no electricity. The list of advantages includes (1) easy to use, (2) convenience, (3) adjustable to suit user's needs, (4) predictable working time (according to battery life span or after recharging), (5) temporary, non-invasive modifications that will not damage the microscope.

Regarding the use of a cellphone flashlight, it turns out that it is not as easy as an emergency light, because in my experience, the cellphone must be held continuously so it does not fall; Apart from that, the light produced by a cellphone flashlight is not as bright as the light from emergency lights. This is understandable because in fact, cell phone flashlights are not designed to produce a specific light beam that is strong enough to shine through the condenser lens. According to Wuben [12] the output of a phone flashlight is estimated around 40 lumens; which is about the same as a 2.5W filament bulb. The type of light is diffused and does not have a concentrated beam spot. Because phone flashlight beams also tend to be more spread, they will be less disturbing to eyesight but in the meantime that means cell phone flashlight is not designed to make sufficient light beam needed for the microscope.

Cellphone flashlights also provide advantages in the field of health examinations [13-15]. The advancement of the high-resolution smartphone camera provides the prospective to alter dramatically the old fashioned but modern table of top fundus camera for photography that have its own limitation [14,15]. For example, of the advantages is the off-label use of smartphones flashlights for indirect retinal photography and videography that made this approach well received ophthalmic clinical practice for its simplicity, portable, contactless and also universality [13-16] which surely augmented real time tele-medical approach for patient care [17].

Smartphone indirect retinal photography necessitates aiming the bright flashlight from the light emitting diode (LED) source available on the rear side of the phone directly on the patient's retina [13,14]. Unfortunately, concerns regarding phototoxic hazards of the bright light, especially with LED lighting, on the already compromised patients' retina raise questions about its safety [18]. A study conducted by Soliman et al. [16] revealed that the LED flashlight of the examined smartphones seemed to be inside the limit of safety when used for indirect smartphone retinal

photography. However, the high configuration of the minuscule wavelength blue light spectrum could be a concern particularly with prolonged and repeated examinations [19].

It is interesting to explore deeper regarding the application (e.g., during completely dark condition) and placement of external light source in order to get the best visual during observation and also while taking photographs, as the last statement is the limitation of this study.

4. CONCLUSION

This simple method study confirm that an external light source can be used for light microscopy analysis whenever there is no electric source available.

ACKNOWLEDGEMENTS

The author would like to thank all the staff in the dept. of Parasitology, Faculty of Medicine for their support in preparing the slides and microscope with all other equipment used in this study

CONSENT AND ETHICAL APPROVAL

It is not applicable.

COMPETING INTERESTS

Author has declared that no competing interests exist.

REFERENCES

1. Maurer MR, Pedrini H, Randi MAF. Processing and visualization of light microscope images. *International Journal of Image and Graphics*. 2011;09. Available:<https://doi.org/10.1142/S0219467809003484>
2. Holgate JH, Webb J. Microscopy | Light Microscopy and Histochemical Methods. In Caballero B (Ed). *Encyclopedia of Food Sciences and Nutrition (Second Edition)*, Academic Press. 2003;3917-3922. ISBN 9780122270550. Available:<https://doi.org/10.1016/B0-12-227055-X/00778-1>
3. Inoué S. Microscope Image Formation. In: *Video Microscopy*. Springer, Boston, MA; 1986. Available:https://doi.org/10.1007/978-1-4757-6925-8_5
4. Lavanya A, Sowmya SV, Rao RS, Augustine D, Haragannavar VC, Nambiar S. Troubleshooters in Light Microscopy. *World J Dent*. 2017;8(6):511-518.

5. Lahiri A (Ed). Chapter 3 - Ray Optics: Optical Systems and Optical Imaging, in Basic Optics, Elsevier. 2016;203-7. ISBN 9780128053577. Available:<https://doi.org/10.1016/B978-0-12-805357-7.00003-4>
6. Evnnett PJ, Hammond CC. Microscopy | Overview. In Worsfold P, Townshend A, Colin Poole C. (Eds). Encyclopedia of Analytical Science (Second Edition), Elsevier. 2005;32-41. ISBN 9780123693976. Available:<https://doi.org/10.1016/B0-12-369397-7/00376-9>
7. Kumari M. Principles of Light Microscopy. Available:<https://maharajacollege.ac.in/fileupload/uploads/60d1b2c08779d20210622095200principles%20and%20application%20of%20light%20microscope.pdf>
8. Goodwin PC. A primer on the fundamental principles of light microscopy: Optimizing magnification, resolution, and contrast. Mol Reprod Dev. 2015 Jul-Aug;82(7-8):502-7. Available:<https://doi.org/10.1002/mrd.22385>
9. Savage B. Keep on operating: how to deal with power cuts. Community Eye Health. 2013;26(84):75.
10. Mukherjee S. The past, present, and future of dentistry through lenses: A short communication. D Y Patil J Health Sci. 2021;9:65-6. Available:https://doi.org/10.4103/dypj.dypj_8_21
11. Compare lumens to watts. LEDified. Available:<https://www.any-lamp.com/lumen-to-watt>
12. Why carry a flashlight when your phone has a torch?. Wuben; 2022 Apr 02. Available:<https://www.wubenlight.com/blog/news/why-carry-a-flashlight-when-your-phone-has-a-torch#:~:text=The%20output%20of%20a%20phone,have%20a%20concentrated%20beam%20spot>
13. Iqbal U. Smartphone fundus photography: A narrative review. Int J Retin Vitr. 2021;7:44. Available:<https://doi.org/10.1186/s40942-021-00313-9>
14. Wintergerst MWM, Petrak M, Li JQ, Larsen PP, Berger M, Holz FG, Finger RP, Krohne TU. Non-contact smartphone-based fundus imaging compared to conventional fundus imaging: A low-cost alternative for retinopathy of prematurity screening and documentation. Sci Rep. 2019 Dec 23;9(1):19711. Available:<https://doi.org/10.1038/s41598-019-56155-x>
15. Panwar N, Huang P, Lee J, Keane PA, Chuan TS, Richhariya A, Teoh S, Lim TH, Agrawal R. Fundus Photography in the 21st Century--A Review of Recent Technological Advances and Their Implications for Worldwide Healthcare. Telemed J E Health. 2016 Mar;22(3):198-208. Available:<https://doi.org/10.1089/tmj.2015.0068>
16. Solyman OM, Hamdy O, Abdelkawi SA, Hassan AA. Investigating the light emitting diode (LED) flashlight characteristics of a sample of smartphones for its safety in indirect retinal photography. Pan Afr Med J. 2022 Sep 8;43:15. Available:<https://doi.org/10.11604/pamj.2022.43.15.32963>
17. Dinh A, Yin AL, Estrin D, Greenwald P, Fortenko A. Augmented Reality in Real-time Telemedicine and Telementoring: Scoping Review. JMIR Mhealth Uhealth. 2023 Apr 18;11:e45464. Available:<https://doi.org/10.2196/45464>
18. Gagné V, Turgeon R. LED Lighting and Retinal Toxicity: A Clearer Picture: LED Lighting and the Reality of Retinal Safety. Curr Trends Ophthalmol and Vis Sci. 2023;2:109. Available:<https://doi.org/10.29011/CTOVS-109.100009>
19. Mainster MA, Findl O, Dick HB, Desmettre T, Ledesma-Gil G, Curcio CA, Turner PL. The Blue Light Hazard Versus Blue Light Hype. Am J Ophthalmol. 2022 Aug;240:51-57. DOI:<https://doi.org/10.1016/j.ajo.2022.02.016>

© 2024 Siagian; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Peer-review history:
The peer review history for this paper can be accessed here:
<https://www.sdiarticle5.com/review-history/111418>



SD Publisher Group

Publisher of peer reviewed international journals, books and monographs

F. No. SDI/IJPR/23/32213

Dated 29th Dec 2023

Subject: Final decision of review process for (Manuscript Number.2023/IJPR/111418) submitted in International Journal of Pathogen Research

Dear Colleague,

We are pleased to inform that peer review process and editorial review process have been completed for your following manuscript

Manuscript Number: 2023/IJPR/111418

Title: "Emergency Microscope light modification by external source in absence of power supply"

Author(s): Forman Erwin Siagian

Acceptance Letter Validation Link: https://acceptance.sciencedomain.org/2023_IJPR_111418.pdf

We are ready with the final decision. We are happy to inform you that your manuscript is officially accepted for publication in International Journal of Pathogen Research

Once your manuscript is moved to publishing, our production editor will keep you informed of your article's progress in the production process. You will also receive a galley proof of your manuscript for final review. We're excited to move forward with your submission. Please feel free to email me with any questions.

Thank you for submitting your paper.

Thanking you.

Dr. M. Basu
Chief Managing Editor



Reg. Offices:

India: Guest House Road, Street no - 1/6, Hooghly, West Bengal, India, Tel: +91 8617752708 | +91 9163821242, WhatsApp: +91 8617752708,
UK: Third Floor, 207 Regent Street, London, W1B 3HH, UK, Fax: +44 20-3031-1429